

E.Z.N.A.[®] FastFilter Plasmid DNA Mini Kit

Isolate high-quality plasmid DNA in just 9 minutes using an innovative lysate clearance column



RAPID

9-minute processing time from bacterial pellet



UNIQUE

Lysate clearance and DNA binding in 1 step



CONVENIENT

FastFilter column eliminates cellular debris pelleting and transfer step



VERSATILE

Process up to 5 mL bacterial cultures with different plasmid types and culture media

E.Z.N.A.[®] FastFilter Plasmid DNA Mini Kit is designed for rapid purification of high-quality plasmid DNA from up to 5 mL of culture following the alkaline-lysis method in just 9 minutes. The kit features an innovative and first-of-its-kind FastFilter mini column nested within a HiBind[®] silica mini spin column to combine lysate clearance and DNA binding into one simple centrifugation step. Following wash and elute steps, purified plasmid DNA is immediately ready for a wide variety of downstream applications such as routine screening, restriction enzyme digestion, transformation, PCR and DNA sequencing.

FASTER PROCESSING WITHOUT SACRIFICING YIELD AND QUALITY

Table 1. Competitor Analysis of Plasmid DNA Purification. pGEM plasmid was purified from cultures (n = 4) using kits from Omega Bio-tek or Company Z or Company Q following manufacturer's recommended centrifugation protocol. Purified Plasmid DNA was eluted at 100 µL irrespective of the manufacturing kit used and quantified using Thermo Scientific's NanoDrop™ 2000c system.

Condition	Culture Volume (mL)	Manufacturer	Yield (µg)	Average A260/A280	Average A260/A230
Minimum Volume Input	0.6	Company Z	2.18	1.92	2.20
		Omega Bio-tek	2.50	1.89	2.20
	1	Company Q	4.45	1.89	2.26
		Omega Bio-tek	4.29	1.88	2.23
Maximum Volume Input	3	Company Z	8.01	1.85	2.31
	5	Omega Bio-tek	18.11	1.85	2.33
	5	Company Q	20.00	1.86	2.28
		Omega Bio-tek	18.11	1.85	2.20

COMPARISON OF PROCESSING TIME FROM BACTERIAL CULTURE

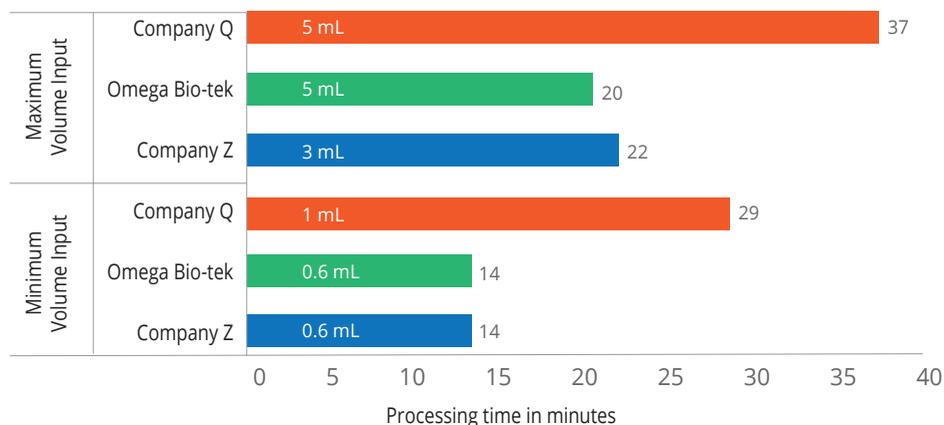


Figure 1. Comparison of Plasmid purification times (n = 4) using kits from Omega Bio-tek or Company Z or Company Q. The processing times shown are actual timed extractions including all pipetting, centrifugation, and bacterial culture pelleting steps. The processing time was comparable using kits from Omega Bio-tek and Company Z at minimum culture volume and was lower by 2 min for Omega Bio-tek at maximum volume. Omega Bio-tek outperformed Company Q with respect to processing time at both the culture volumes tested.



innovations in nucleic acid isolation

Omega Bio-tek, Inc.
400 Pinnacle Way, Suite 450
Norcross, GA 30071

Phone: 770-931-8400
Email: info@omegabiotek.com
Web: www.omegabiotek.com



© 2022 Omega Bio-tek, Inc. All rights reserved. E.Z.N.A., E-Z.96 and Mag-Bind are trademarks of Omega Bio-tek, Inc. All other trademarks and trade names are the property of their respective holders. For research use only.

E.Z.N.A.[®] FastFilter Plasmid DNA Mini Kit

Isolate high-quality plasmid DNA in just 9 minutes using an innovative lysate clearance column

HIGH-QUALITY PLASMID DNA SUITABLE FOR SEQUENCING REACTIONS

Table 2. Plasmid DNA purified using the E.Z.N.A. FastFilter Plasmid DNA Mini Kit was used in a 5 µL Sanger sequencing reaction. The sequencing reaction was analyzed on an Applied Biosystems 3730XL. The samples had an average CRL of 994 bp and an average QV20+ of 985 with a quality score greater than 20 ($\leq 1\%$ probability of error in base calling).

Sample ID	Quality Score	Contiguous Read Length (CRL)	QV20+	Average Intensity
1	45	987	979	2692.5
2	46	993	977	2181
3	46	1002	1001	2650.3

VERSATILITY USING DIFFERENT PLASMID TYPES AND CULTURE MEDIA

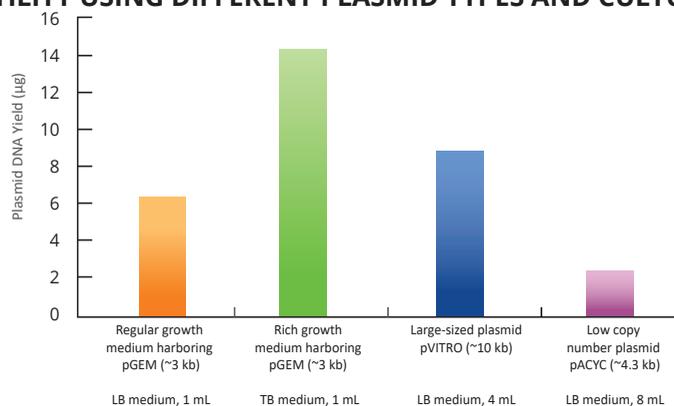


Figure 2. E.Z.N.A.[®] FastFilter Plasmid DNA Mini Kit is capable of handling diverse sample input conditions ranging from plasmid types, culture medium as well as input culture volume. The plasmid yield may vary based on these conditions.

COMPLETE DIGESTION WITH VARIOUS RESTRICTION ENZYMES

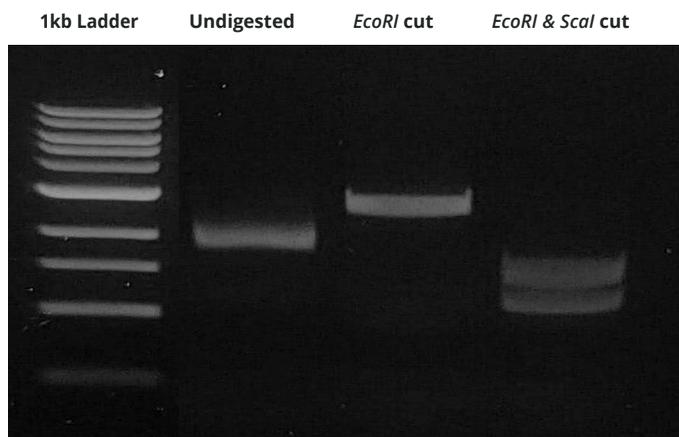


Figure 3. pGEM plasmid DNA from overnight bacterial cultures was purified using the E.Z.N.A. FastFilter Plasmid DNA Mini Kit and analyzed by restriction digestion. Complete digestion was observed for the various restriction enzymes tested.

HIGH-QUALITY, SUPERCOILED PLASMID DNA

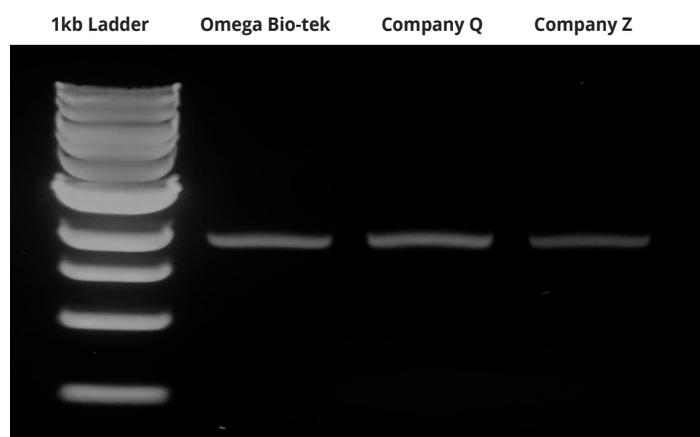


Figure 4. Plasmid DNA Quality Assessment using kits from Omega Bio-tek or Company Q or Company Z. No genomic DNA was present on the agarose gel and plasmid DNA appears supercoiled.

Product Description	Preps	Cat No.
E.Z.N.A. [®] FastFilter Plasmid DNA Mini Kit	10	D6944-00
	100	D6944-01
	300	D6944-02